



## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<b>(51) International Patent Classification <sup>5</sup> :</b>  <b>A61M 29/00</b>	<b>A1</b>	<b>(11) International Publication Number:</b> <b>WO 93/06883</b>  <b>(43) International Publication Date:</b> 15 April 1993 (15.04.93)
<b>(21) International Application Number:</b> PCT/US92/07794 <b>(22) International Filing Date:</b> 15 September 1992 (15.09.92) <b>(30) Priority data:</b> 771,013                      2 October 1991 (02.10.91)                      US <b>(71) Applicant:</b> TARGET THERAPEUTICS, INC. [US/US]; 47201 Lakeview Boulevard, P.O. Box 5120, Fremont, CA 94537-5120 (US). <b>(72) Inventors:</b> CHEE, U., Hiram ; 4151-D El Camino Way, Pa- lo Alto, CA 94306 (US). MARIANT, Mike ; 2160 Ventu- ra Place, Santa Clara, CA 95051 (US). <b>(74) Agents:</b> WHEELLOCK, E., Thomas et al.; Morrison & Fo- erster, 755 Page Mill Road, Palo Alto, CA 94303-1018 (US).		<b>(81) Designated States:</b> AU, CA, CS, FI, HU, JP, KR, NO, Eu- ropean patent (AT, BE, CH, DE, DK, ES, FR, GB, GR, IE, IT, LU, MC, NL, SE).  <b>Published</b> <i>With international search report.</i>
<b>(54) Title:</b> VASOOCCLUSION COIL WITH ATTACHED FIBROUS ELEMENT(S)  <div style="text-align: center;"> </div>		
<b>(57) Abstract</b>  A device for occluding a blood vessel comprising a helical metal coil (11) having at least one fibrous element (12) attached to its proximal end (18) wherein the fibrous element(s) (12) extends in a sinusoidal wave configuration, the loops (19) of which extend about individual windings (13) at spaced intervals along the axis of the coil (11).		

**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	FR	France	MR	Mauritania
AU	Australia	GA	Gabon	MW	Malawi
BB	Barbados	GB	United Kingdom	NL	Netherlands
BE	Belgium	GN	Guinea	NO	Norway
BF	Burkina Faso	GR	Greece	NZ	New Zealand
BG	Bulgaria	HU	Hungary	PL	Poland
BJ	Benin	IE	Ireland	PT	Portugal
BR	Brazil	IT	Italy	RO	Romania
CA	Canada	JP	Japan	RU	Russian Federation
CF	Central African Republic	KP	Democratic People's Republic of Korea	SD	Sudan
CG	Congo	KR	Republic of Korea	SE	Sweden
CH	Switzerland	LI	Liechtenstein	SK	Slovak Republic
CI	Côte d'Ivoire	LK	Sri Lanka	SN	Senegal
CM	Cameroon	LU	Luxembourg	SU	Soviet Union
CS	Czechoslovakia	MC	Monaco	TD	Chad
CZ	Czech Republic	MG	Madagascar	TG	Togo
DE	Germany	ML	Mali	UA	Ukraine
DK	Denmark	MN	Mongolia	US	United States of America
ES	Spain			VN	Viet Nam
FI	Finland				

5        VASOOCCLUSION COIL WITH ATTACHED FIBROUS ELEMENT(S)DescriptionTechnical Field

10                This invention is in the field of vasoocclusion devices. More particularly it relates to a vasoocclusion coil to which fibrous elements are attached.

Background

15                Vasoocclusion devices are surgical implements that are placed within vessels, typically via a catheter to block the flow of blood through the vessel. One type of vasoocclusive device is a helical wire coil that has windings that are dimensioned to engage the walls of the  
20        vessels. Fibers are laid crosswise through the windings to provide a substrate for embolization within the vessel. Coils of such structure are available commercially from Cook, Inc.

              U.S. 4,994,069 describes a vasoocclusive coil  
25        that assumes a linear helical configuration when stretched and a folded convoluted configuration when relaxed. The stretched condition is used in placing the coil at the desired site and the coil assumes its relaxed configuration--which is better suited to occlude the  
30        vessel--once the device is so placed.

              A principal object of the present invention is to provide a helical vasoocclusion coil to which fibrous elements are attached in a manner that ensures they will

35

-2-

not be dislodged from the coil and enhances the ability of the coil to facilitate embolization.

#### Disclosure of the Invention

5           The invention is a vasoocclusive device comprising:

(a) a helical coil having a multiplicity of windings extending between a first end and a second end;

10           (b) at least one fibrous element having a first end attached to one of said windings in the region of the first end of the coil, a second end attached to another of said windings in the region of the second end of the coil, with the portion of the element intermediate said ends extending axially along the coil in a generally  
15           serpentine configuration composed of a plurality of loops having maxima that extend radially outwardly and minima that extend radially inwardly and are threaded about individual windings at spaced intervals along the coil.

#### 20           Brief Description of the Drawings

Fig. 1 is a fragmentary elevational view (not to scale) of one embodiment of the invention.

Fig. 2 is a fragmentary elevational view (not to scale) of another embodiment of the invention.

25           In the drawings, like structures are referred to by the same reference numeral.

#### Modes for Carrying Out the Invention

30           Fig. 1 depicts one embodiment, generally designated 10, of the vasoocclusive coil of the invention. The device 10 has two components: a helical coil 11; and a fibrous element 12.

35           Coil 11 will typically be made of a radiopaque material such as platinum, tungsten or gold wire. The

diameter of the wire will usually be in the range of 0.05 to 0.25 mm. The coil has a multiplicity of individual windings 13. The axial length of the coil will usually be in the range of 0.2 to 100 cm, more usually 0.2 to 40  
5 cm and the diameter of the coil will normally be 0.015 to 0.1 cm, more usually 0.025 to 0.1 cm. The coil will typically have about 10 to 70 windings per cm, more typically about 10 to 40 windings per cm.

The fibrous element 12 may be a bundle of  
10 individual fibers 14 (typically 5 to 100 fibers per bundle, preferably 20 to 30 fibers per bundle) as shown in Fig. 1 or a monofilament 15 as shown in Fig. 2. The fibers may be made from biocompatible materials such as Dacron (polyethyleneterephthalate), polyglycolic acid,  
15 polyactic acid, fluoropolymer (polytetrafluoroethylene), nylon (polyamide), or silk.

In embodiment 10, end 16 of the bundle is tied to winding 17 of the coil by a knot 18. Knotting at the ends of the bundle is desirable, but not essential, as  
20 the threading of the loops about the windings (see below) is sufficient to anchor the bundle to the coil. The specific location of attachment of end 16 is not critical and it will typically be either at the proximal end 18 of the coil or at a site on the coil spaced from the  
25 proximal end a distance greater than the loop length (see below) when the loop is lying flat on the coil. The fiber bundle extends in a generally serpentine or sinusoidal wave configuration along the exterior of the coil in a series of outer-directed (relative to the coil  
30 axis) loops 19 and inner-directed loops 20. The inner-directed loops are threaded about individual windings, designated 21, 22, 23 and 24 at spaced intervals (indicated as distance "a" between knot 18 and winding  
21) along the coil. In Fig. 1, the individual windings

-4-

are shown in a slightly expanded (spaced) condition for the purposes of illustration. More normally, however, the windings will be closer together so that the windings on either side of windings 21, 22, 23 and 24 pinch the fiber bundle against windings 21, 22, 23 and 24. The length of the intervals ("a") between the windings about which the fiber bundle passes may vary. It will typically be about 0.05 to 1 cm. The interval spacing may be the same or different along the length of the coil. Correspondingly, the loop length (e.g., the curvilinear length of the bundle from knot 18 to winding 21) may vary and may be the same or different from loop-to-loop. The loop length will normally be 0.1 to 2 cm, more usually 0.1 to 0.5 cm.

The fibrous element will usually extend between about 10% to 90% of the total axial length of coil. In other words the axial distance over which the element extends will usually be 0.05 to 90 cm, more usually 0.05 to 15 cm. (The dashed lines in the drawings indicate that the coil extends distally.) The element will typically be located at the proximal end of the wire. In this regard, the term "proximal" is relative to orientation in which the coil is loaded within a catheter. The distal end of the element is affixed by knot 25 to winding 26.

While Fig. 1 depicts a coil with only a single affixed fiber bundle, it will be appreciated that a multiplicity (typically 2 to 4) of fiber bundles may be similarly attached at spaced intervals about the circumference of the coil.

Fig. 2 illustrates another embodiment, generally designated 30, of the vasoocclusive device of the invention. There are two differences between device 10 and device 30: (1) the fibrous element in Fig. 2 is a

-5-

monofilament 15 and (2) there are two monofilaments 15 attached to the coil rather than a single fibrous element. As shown, the two monofilaments are spaced approximately 180° apart about the circumference of the coil. As in the case of device 10, additional monofilaments 15 may be affixed to the coil if desired.

The vasoocclusion coils of this invention are used in a manner similar to the coil of U.S. 4,994,069. Briefly, the coil is preferably supplied in prepackaged form in a sterile cannula which is adapted to engage the proximal end of a catheter. In this regard the loops of the fibrous bundle will be pressed flat against the coil for placement in the cannula and catheter. Once the catheter is in place within a vessel, the coil-containing cannula is placed into engagement with the proximal end of the catheter and the coil is transferred from the cannula lumen into the catheter lumen by exerting force on the proximal end of the coil. A pusher rod is used to push the coil through the catheter to the desired coil release site. The location of the coil may be visualized due to the radiopacity of the helical coil. Once at the site, the coil is plunged from the catheter lumen into the vessel. This allows the flexible fiber loops to extend outwardly from the coil surface to fill the vessel.

Modifications of the above-described modes for carrying out the invention that are obvious to those of skill in the fields of medical device design generally, and vasoocclusion specifically are intended to be within the scope of the following claims.

Claims

1. A vasoocclusive device comprising:
  - (a) a helical coil having a multiplicity of  
5 windings extending between a first end and a second end;
  - (b) at least one fibrous element having a first  
end and a second end, with the portion of the element  
intermediate said ends extending axially along the coil  
in a generally serpentine configuration composed of a  
10 plurality of loops having maxima that extend radially  
outwardly and minima that extend radially inwardly and  
are threaded about individual windings at spaced  
intervals along the coil.
- 15 2. The device of claim 1 wherein the helical  
coil is from 2 to 100 cm in length, 0.015 to 0.1 cm in  
diameter and has about 100 to 70 windings per cm.
- 20 3. The device of claim 2 wherein the fibrous  
element is attached to the proximal end of the helical  
coil and extends over about 10% to 90% of the length of  
the coil.
- 25 4. The device of claim 1 wherein there are a  
multiplicity of fibrous elements.
5. The device of claim 1 wherein there are 1  
to 4 fibrous elements.
- 30 6. The device of claim 1 wherein the fibrous  
element is a bundle of individual fibers.
- 35 7. The device of claim 1 wherein the fibrous  
element is a monofilament.

-7-

8. The device of claim 1 wherein the length of an individual loop is 0.1 to 2 cm.

9. The device of claim 1 wherein said spaced interval is about 0.05 to 1 cm in length.

10. The device of claim 8 wherein said spaced interval is about 0.05 to 1 cm in length.


11. The device of claim 10 wherein the fibrous element is a bundle of about 5 to 100 individual fibers, there are 1 to 4 fibrous elements, the length of the helical coil is 2 to 100 cm, the fibrous elements are affixed to the proximal end of the helical coil, and the fibrous elements extend over about 25% to 50% of the length of the coil.

12. The device of claim 1 wherein the first end of the fibrous element is attached to one of said windings in the region of the first end of the coil and the second end is attached to another of said windings.


13. The device of claim 11 wherein the first end of the fibrous element is attached to one of said windings in the region of the first end of the coil and the second end is attached to another of said windings.

30

35

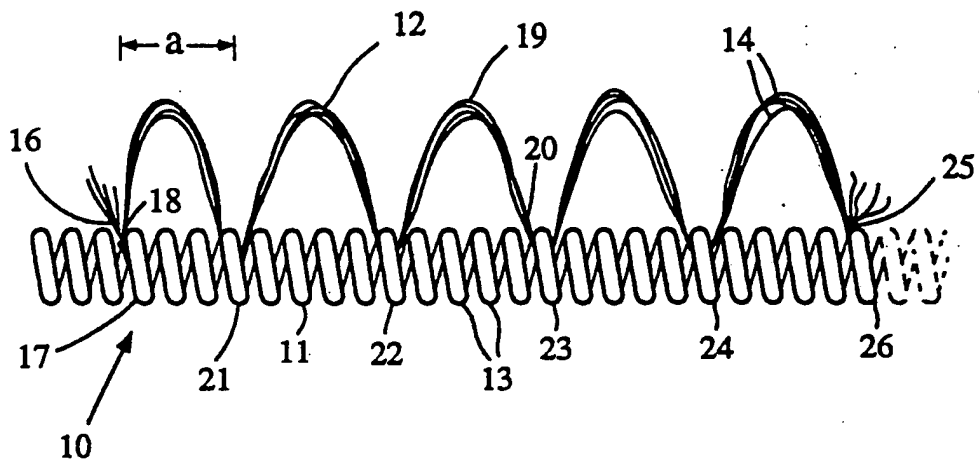

**Figure 1**

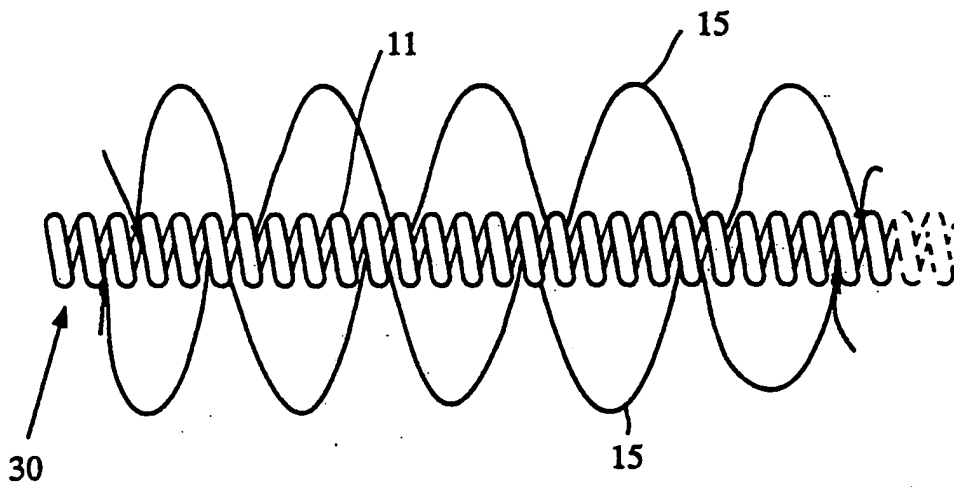

**Figure 2**

## INTERNATIONAL SEARCH REPORT

International application No.  
PCT/US92/07794

## A. CLASSIFICATION OF SUBJECT MATTER

IPC(5) :A61M 29/00

US CL :606/191, 198; 604/104

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

U.S. : 606/191, 198; 604/104, 606/194, 200; 623/1, 11, 12

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)  
none

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
<u>X</u> Y	US, A, 4,994,069 (RITCHART ET AL.) 19 February 1991, see col. 2, lines 1-10.	<u>1</u> 2-13
A	US, A, 4,830,003 (WOLFF ET AL.) 16 May 1989, see Fig. 4 and Abstract.	1-13
A	US, A, 4,718,907 (KARWOSKI ET AL.) 12 January 1988, see Fig. 2 and Abstract.	1-13
A,P	US, A, 5,071,407 (TERMIN ET AL.) 10 December 1991, see Figs. 3-9 and Abstract.	1-13



Further documents are listed in the continuation of Box C.



See patent family annex.

## \* Special categories of cited documents:

"A" document defining the general state of the art which is not considered to be part of particular relevance

"E" earlier document published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T"

later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X"

document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y"

document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"Z"

document member of the same patent family

Date of the actual completion of the international search

28 OCTOBER 1992

Date of mailing of the international search report

9 DEC 1992

Name and mailing address of the ISA/ US  
Commissioner of Patents and Trademarks  
Box PCT  
Washington, D.C. 20231

Facsimile No. NOT APPLICABLE

Authorized officer

C.A. BENNETT

Telephone No. (703) 308-0980

*Nguyen*  
NGUYEN NGOC-HO  
INTERNATIONAL DIVISION